



# resDetect™ resDNA Sample Preparation Kit (Magnetic Beads)

Catalog Number: OPA-R005

Assay Tests: 50 Preps

For Research Use Only. Not For Use in Diagnostic or Therapeutic Procedures

**IMPORTANT: Please carefully read this user guide before performing your experiment.**

## **Product Information**

The resDNA Sample Preparation Kit is designed for extraction of residual DNA (resDNA) from biopharmaceuticals. Use the kit before you detect resDNA from test samples. For detection information, see the resDNA Quantitation Kit User Guide ([ACROBiosystems.com](https://www.acrobiosystems.com)).

This kit is isolate DNA from a sample using magnetic beads. The process typically involves lysing the sample to release the DNA, then using magnetic beads coated with a DNA-binding agent to selectively bind the DNA. The beads are then separated from the mixture using a magnetic stand, and the DNA can be washed and eluted off the beads for further analysis or use. This method is often preferred over traditional methods due to its high efficiency and ease of use.

## Contents and Storage

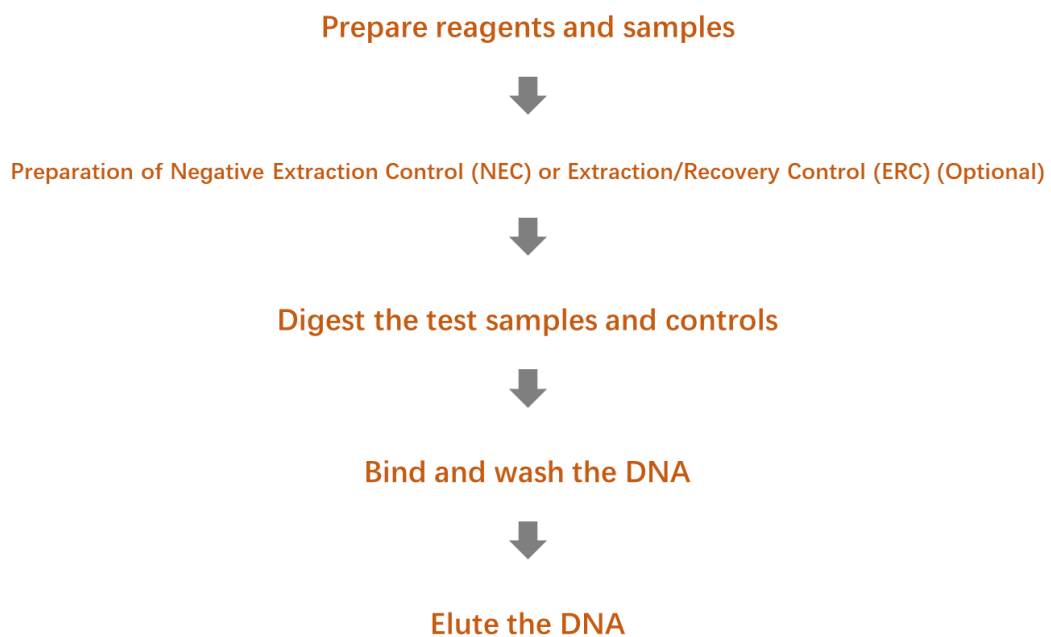
The kit can be used for 50 preps of DNA extraction from test samples.

Contents	Amount	Storage
Buffer NT	1.5 mL	10°C to 30°C  <b>Note:</b> The Proteinase K and MagBeads Suspension can be stored in ambient temperature (10 to 30°C). For optimal long-term stability, these two components are recommended to be stored in 2-8°C
Buffer LA	1.5 mL	
Buffer LB	24 mL	
Proteinase K	4 mL	
MagBeads Suspension (MB)	1.5 mL	
CR Powder	310 µg	
Buffer WA	38 mL	
Buffer WB	18 mL	
Buffer EB	6 mL	
1X PBS	10 mL	

The unopened kit is stable for 12 months from the date of manufacture if stored at 10°C to 30°C.

**Required materials not supplied.**

<b>Equipments</b>	Magnetic stand
	Block heater
	Mini centrifuge
	Vortex
	Pipettors: P1000, P200, P100, P10
<b>Reagents</b>	Isopropanol, 99.7%
	Ethanol, 99.7%
	1X PBS (free of Mg <sup>2+</sup> and Ca <sup>2+</sup> ) or 1×TE (pH7.0~pH8.0) as sample dilution buffer
	DNase/RNase-free ddH <sub>2</sub> O
<b>Consumables</b>	Disposable gloves
	Nuclease-free, DNA-free aerosol-resistant pipet tips
	Low DNA-Binding Microcentrifuge Tubes (Nuclease-free, DNA-free)

**Workflow**

## Prepare the reagents and samples.

### Prepare the reagents: before first use of the kit.

1. Incubate the MagBeads Suspension at room temperature for 30 mins, or until the beads are completely suspended.
2. Refer to the bottle label, add amount of 99.7% ethanol to bottle of Buffer WA or WB, then mix completely.
3. Label the bottle to indicate that it contains ethanol, then store the bottle at room temperature.
4. Preparation of CR Solution: Briefly centrifuge the CR Powder tube, then add 310  $\mu\text{L}$  DNase/RNase-free ddH<sub>2</sub>O to the tube, and vortex thoroughly.

**NOTE:** *The CR Solution should be stored at -20°C, it can be divided into small portions to avoid freeze-thaw cycles.*

### Prepare the samples.

#### Sample dilution (if necessary)

Test samples from the early purification process often contain levels of DNA that are above the highest point of the assay standard curve. You must dilute these samples (from 1:10 up to 1:1,000) before sample preparation.

1. Dilute test samples before DNA extraction with sample dilution buffer. Please use 1X PBS (free of Mg<sup>2+</sup> and Ca<sup>2+</sup>) or 1 X TE (pH7.0~pH8.0) as sample dilution buffer.
2. For the powder testing samples, please resolve the samples with sample dilution buffer.

## Prepare the NEC and ERC. (Optional)

### Preparation of Negative Extraction Control (NEC)

A Negative Extraction Control (NEC) omits any DNA template from a reaction. This control is used to monitor contamination during nucleic acid extraction. In cases where large numbers of DNA samples need extracted, it is recommended that negative extraction controls are included between the samples for testing.

1. Label low DNA-binding 1.5 mL microfuge tubes "NEC".
2. Add **100 µL** of 1X PBS (free of Mg<sup>2+</sup> and Ca<sup>2+</sup>) or 1×TE (pH7.0~pH8.0) to each tube.

**Note:** *NEC should be the same as sample dilution buffer (If used in the process sample dilution).*

### Preparation of Extraction/Recovery Control (ERC) (Optional)

You can use an Extraction/Recovery Control (ERC) to assess the efficiency of DNA extraction, recovery, and quantitation from test samples. Additionally, you can use ERC to verify assay and system performance.

**Note:** Adjust the amount of Target residual DNA control added to the sample for those test samples that contain higher background levels of DNA. To ensure accurate results, the amount of Target residual DNA control that you add to a test sample should be approximately two to three times the amount of DNA measured in the test sample without the addition of the Target residual DNA control. To calculate the efficiency of DNA recovery and quantitation from the test samples, subtract the amount of DNA measured in the sample without the addition of Target residual DNA control from the amount of DNA measured in the ERC sample.

To learn about the procedure preparing ERC sample containing Target residual DNA control per well for qPCR analysis, refer to the corresponding User Guide of resDNA Quantitation Kit ([ACROBiosystems.com](https://www.acrobiosystems.com)).

### Digest the test samples and controls.

1. Label low DNA-binding 1.5/2.0mL microfuge tubes "Sample", "NEC".
2. Add 100  $\mu$ L of samples and controls to each tube.
3. Add 22  $\mu$ L of Buffer NT, 70  $\mu$ L of Proteinase K and 25  $\mu$ L of Buffer LA to each tube, briefly vortex and centrifuge.
4. Incubate at 56°C for 30 mins on a block heater, with vortexing at 1000 rpm. If available, set heater lid to 70°C.
5. Briefly centrifuge, and cool samples to room temperature.
6. Add 400  $\mu$ L of Buffer LB to each tube, then close the cap and invert five times to mix.
7. Vortex 1 min and briefly centrifuge.

### Bind the DNA

1. Add 180  $\mu$ L of isopropanol, 25  $\mu$ L of MagBeads Suspension and 3  $\mu$ L of CR Solution to each tube, then close the cap and invert five times to mix.

**NOTE:** The MagBeads Suspension should be resuspended before use.

2. Vortex all the tubes for 1 min.
3. Let the tubes stand for 5 mins, and then vortex for 30 seconds.
4. Repeat the step 3.
5. Briefly centrifuge and place the tubes in the magnetic stand with the pellet against the magnet, then let the tubes stand for 5 mins or until the solution is clear.
6. Without disturbing the magnetic beads, remove the supernatant using a pipette or by aspiration.

### Wash the DNA

1. Add 700  $\mu$ L Buffer WA to each tube, then vortex for 10 seconds.
2. Briefly centrifuge the tubes, then place the tubes in the magnetic stand, let the tubes stand for 2 mins or until the solution is clear.
3. Without disturbing the magnetic beads, remove the supernatant using a pipette or by aspiration.

4. Repeat the steps 1-3.
5. Add 700  $\mu\text{L}$  Buffer WB to each tube, then vortex for 10 seconds.
6. Repeat the steps 2-3.
7. Use a P10 to remove the remaining solution from the bottom of the tube.
8. With the tube lid open, air-dry the Magnetic beads in the magnetic stand for no more than 5 minutes at room temperature.

**Note:** Do not over-dry; the bonded DNA are not easily eluted from the over-dried beads.

### Elute the DNA

1. Add 50-100  $\mu\text{L}$  of Buffer EB to each tube, then resuspend the beads by vortexing or pipetting up and down until suspension is fully homogenized.
2. Incubate the tubes at 70°C for 10 mins on a block heater, with vortexing at 1000 rpm.
3. Briefly centrifuge the tubes for 15 seconds, then place the tubes in the magnetic stand, let the tubes stand for 2-5 mins or until the solution is clear.
4. Use a P100 to transfer the liquid phase to a new 1.5 mL microcentrifuge tube.

**Note:** Do not disturb the magnetic beads.

The purified, high-quality eluted DNA is ready to use in demanding downstream applications.

Store eluted DNA for up to 24 hours at 2°C to 8°C or for long time at -20°C.